

The logo for Revvity, featuring the word "revvity" in a white, lowercase, sans-serif font on a black background. The logo is positioned in the upper right corner of the page, partially overlapping a decorative graphic of overlapping, translucent yellow and orange spheres.

revvity

USER MANUAL

OM100 Ultrasonic Homogenizer

Version: BC

Date: October 2024

Document Number: 03-2021-100

Data herein has been verified and validated. It is believed adequate for the intended use of the instrument. If the instrument or procedures are used for purposes over and above the capabilities specified herein, confirmation of the validity and suitability should be obtained; otherwise Revvity does not guarantee results and assumes no obligation or liability. This publication is not a license to operate under, or a recommendation to infringe upon, any process patents.

This product is warranted to be free from defects in material and workmanship for a period of ONE YEAR from the date of delivery. Ultrasonic probes are guaranteed against defects for a period of ONE YEAR from date of shipment. A defective probe will be replaced once without charge, if failure occurs within the warranty period. Wear resulting from cavitation erosion is a normal consequence of ultrasonic processing and is not covered by this warranty.

Revvity will repair or replace and return free of charge any part which is returned to its factory within said period, transportation prepaid by user, and which is found upon inspection to have been defective in materials or workmanship. This warranty does not include normal wear from use; it does not apply to any instrument or parts which have been altered by anyone other than an employee of Revvity nor to any instrument which has been damaged through accident, negligence, failure to follow operating instructions, the use of electric currents or circuits other than those specified on the plate affixed to the instrument, misuse, or abuse. Revvity reserves the right to change, alter, modify, or improve any of its instruments without any obligation whatever to make corresponding changes to any instrument previously sold or shipped.

THE FORGOING OBLIGATION IS IN LIEU OF ALL OBLIGATIONS AND LIABILITIES INCLUDING NEGLIGENCE AND ALL WARRANTIES OF MERCHANTABILITY OR OTHERWISE, EXPRESSED OR IMPLIED IN FACT OR BY LAW, AND STATE OUR ENTIRE AND EXCLUSIVE LIABILITY AND BUYERS EXCLUSIVE REMEDY FOR ANY CLAIM OF DAMAGES IN CONNECTION WITH THE SALE OR FURNISHING OF GOODS OR PARTS, THEIR DESIGN, SUITABILITY FOR USE, INSTALLATION, OR OPERATION. REVVITY WILL IN NO EVENT BE LIABLE FOR ANY SPECIAL OR CONSEQUENTIAL DAMAGES WHATSOEVER, AND THEIR LIABILITY UNDER NO CIRCUMSTANCES WILL EXCEED THE CONTRACT PRICE FOR THE GOODS FOR WHICH LIABILITY IS CLAIMED.

This product has been engineered for safety; however, basic safety precautions and common sense must always be demonstrated when using any electrical product.

High voltage is present in the generator (power supply), converter and high frequency cable. There are no user-serviceable parts inside any of these devices.

- **DO NOT** attempt to remove the generator cover or converter case.
- **DO NOT** touch any open cable connections on the unit while the power is turned ON.
- **DO NOT** operate generator with converter disconnected from high voltage cable. High voltage is present in the cable and may pose a shock hazard.
- **DO NOT** attempt to disconnect the converter high voltage cable while the unit is running.
- **DO NOT** allow the tip of a vibrating horn or probe to touch the counter top or any other hard surface. It could damage the probe, overload the generator, or damage the surface.
- **DO NOT** operate unit with a damaged cable. Doing so may cause serious injury.
- **DO NOT** turn off Main power switch while running a probe. Stop sonication by lowering intensity setting knob to 0 or release thumb switch.
- **NEVER** immerse the converter in liquids of any kind, or let condensed moisture or liquid drip into the converter.
- **NEVER** grasp an activated horn or touch the tip of a vibrating probe. It can cause severe burns and tissue damage.
- **NEVER** allow a probe to vibrate in air.
- **NEVER** hold or clamp the converter by the front driver or by the horn itself. This can cause permanent damage to the system. Support the converter by only clamping around the converter housing (upper portion).

- Avoid touching the bottom or sides of a sample vessel with an activated probe. It may crack or shatter the glass or melt the plastic. Use glassware that is free from cracks or chips.
- Turn OFF the power switch, unplug the generator and disconnect the power cord from the back of the generator before attempting to replace the fuses.
- Inspect high frequency cable for cracks in the protective outer jacket.
- The generator must be properly grounded with a 3-prong plug. Test electrical outlet for proper grounding prior to plugging in unit.
- Install the OM100 Ultrasonic Homogenizer in an area free from excessive dust, dirt, explosive or corrosive fumes and protected from extremes in temperature and humidity. Do not place the Generator within a Fume Hood.
- Hearing protection is highly recommended. It is recommended that a sound abating enclosure or ear protection be used when operating the OM100 Ultrasonic Homogenizer
- In case of AC power loss, wait 3 minutes minimum before reapplying power.

Copyright

This manual is published by Revvity 935 Cobb Place Blvd, Kennesaw, GA 30144 USA. Copyright Revvity, Inc. All rights reserved, including but not limited to those rights to reproduce this publication or parts thereof. Reproduction of this publication or parts thereof, or the products it describes, by any means or in any form is expressly prohibited without the written permission of Revvity.

Trademarks

Revvity is a registered trademark of Revvity. All other trademarks are the property of their respective owners.

Proper Equipment Operation

To reduce the risk of electric shock, do not remove the cover. No user serviceable parts are inside. Refer to qualified service personnel if help is required.

Use this product only in the manner described in this manual. If the equipment is used in a manner not specified by the manufacturer, the protection provided by the equipment may be impaired.

Cleaning

Follow internal laboratory process for cleaning and decontamination using 70% ethanol followed by a disinfecting wipe, then a final rinse with ethanol.

Preventative Maintenance

Normal use: 12 month interval.

Operating Environment

39°F to 104°F / 5°C to 40°C, Humidity: 10% to 95% RH. Internal use only

Electrical Supply

90-230V, 50/60 Hz, 4A Max

FCC

This device complies with part 15 of the FCC (United States Federal Communications Commission) Rules. Operation is subject to the following two conditions:

- This device may not cause harmful interference, and
- This device must accept any interference received, including interference that may cause undesired operation.

CE/UKCA












This device complies with all CE and UKCA rules and requirements.

Changes or modifications to this equipment not expressly approved by the party responsible for compliance could void the user's authority to operate the equipment.

Table of Contents

Table of Symbols.....	5
Specifications.....	6
Principles of Operation.....	7
Relationship of Amplitude and Wattage	7
System Overview	9
Functions Key Controls and Connectors.....	10
Convertor Clamping.....	11
Preparation for Use	12
Inspection	12
Electrical Requirements	12
Installing the OM50 Ultrasonic Homogenizer	12
Operating Instructions	13
Setup.....	13
Operation - Amplitude	14
Operation - Timer	14
Operation - Pulser.....	15
Operation - Review	15
Maintenance.....	16
Probe Maintenance.....	16
Attaching and Detaching Probes	16
System Cleaning Instructions.....	17
Troubleshooting.....	17
Overload Condition	17
Frequently Asked Questions	18
Probe Size versus Sample Volume.....	18
How to Prevent Foaming (Small Sample Issue).....	18
Tip depth.....	18
Power versus Intensity.....	19
Viscosity Limitations.....	19
Keeping Samples Cool.....	19
Accessories	20
Appendix.....	21
Transport and Storage	21
Equipment Disposal.....	21

Table of Symbols

Symbol	Description	Symbol	Description
	Caution. Refer to the User documentation (ISO 7000-0434B)		On (power). (IEC 60417-5007)
	Hazardous voltage; risk of electric shock. (IEC 60417-6042)		Off (power). (IEC 60417-5008)
	Fuse. (IEC 60417-5016)		Consult Instructions for Use. (ISO 7000-1641)
	Alternating current. (IEC 60417-5032)		CE Compliance Mark
	UKCA Certification Mark		WEEE symbol (EN50419:2005)
	RoHS Certification Mark		

Specifications

Part Number	29-060-100-120 and 29-060-100-220
Power Supply	
Input Voltage	108 to 132 VAC @ 50/60 Hz and 198 to 264 VAC @ 50/60 Hz
Rated Current	2.4 Amps Max and 1.2 Amps Max
Fuse Rating	3 Amps Slow Blow and 1.6 Amps Slow Blow
Output Voltage	380 VRMS
Output Frequency	20 KHz
Rated Power	100 Watts
Weight	7 lbs. (3.2 kg)
Dimensions	W: 8" (20.3 cm), D: 13.75" (34.9 cm), H: 5.75" (14.6 cm)
Convertor	
Weight	0.75 lbs. (0.34 kg)
Dimensions	L: 6" (15.0 cm) x W: 1.25" (3.0 cm)
Materials	Aluminum Alloy
Environmental	
Pollution Degree	2
Overvoltage Category	II
Temperature	39°F to 104°F / 5°C to 40°C
Relative Humidity	10 to 95% (Non Condensing)
Altitude	6,651 ft. (2000 m)
Warranty	1 Year
Standards Approval	CE and UKCA Approved
Other	For Indoor Use Only

The power cord supplied with the OM100 Ultrasonic Homogenizer must be used.

If the 220V plug is not configured to match the wall receptacle, a properly grounded universal AC socket adapter must be added.

IMPORTANT: Universal adapters do not convert voltage or frequency. Manufacturer is not responsible for damage caused by the use of an improper power cord or adapter. Transformers are not recommended.

Principles of Operation

The OM100 ultrasonic power supply transforms AC line power to a 20 KHz signal that drives a piezoelectric converter/transducer. This electrical signal is converted by the transducer to a mechanical vibration due to the characteristics of the internal piezoelectric crystals.

The vibration is amplified and transmitted down the length of the horn/probe where the tip longitudinally expands and contracts. The distance the tip travels is dependent on the amplitude selected by the user through the keypad. As you increase the amplitude setting the sonication intensity will increase within your sample.

In liquid, the rapid vibration of the tip causes cavitation, the formation and violent collapse of microscopic bubbles. The collapse of thousands of cavitation bubbles releases tremendous energy in the cavitation field. The erosion and shock effect of the collapse of the cavitation bubble is the primary mechanism of fluid processing.

The probe tip diameter dictates the amount of sample that can be effectively processed. Smaller tip diameters probes deliver high intensity sonication, but the energy is focused within a small, concentrated area. Larger tip diameters can process larger volumes but offer lower intensity.

The choices of a power supply and horns/probes are matched to the volume, viscosity, and other parameters of the application. Horns are available for both direct and indirect sonication.

Relationship of Amplitude and Wattage

Sonication power is measured in watts. Amplitude is a measurement of the excursion of the tip of the probe (a probe is also known as a horn).

Some ultrasonic homogenizers have a wattage display. During operation, the wattage displayed is the energy required to drive the radiating face of a probe, at that amplitude setting against a specific load, at that moment. For example, the unit experiences a higher load when processing viscous samples than when compared to aqueous samples.

The speed/cruise control on an automobile can, to a certain extent, be compared to an ultrasonic homogenizer. The speed/cruise control is designed to ensure that the vehicle maintains a constant rate of travel. As the terrain elevations change, so do the power requirements. The cruise control senses these requirements and automatically adjusts the amount of power delivered by the engine to compensate for these ever-changing conditions. The greater the terrain rate of incline and resistance to the vehicle's movement, the greater the amount of power delivered by the engine to overcome that resistance and maintain a constant speed.

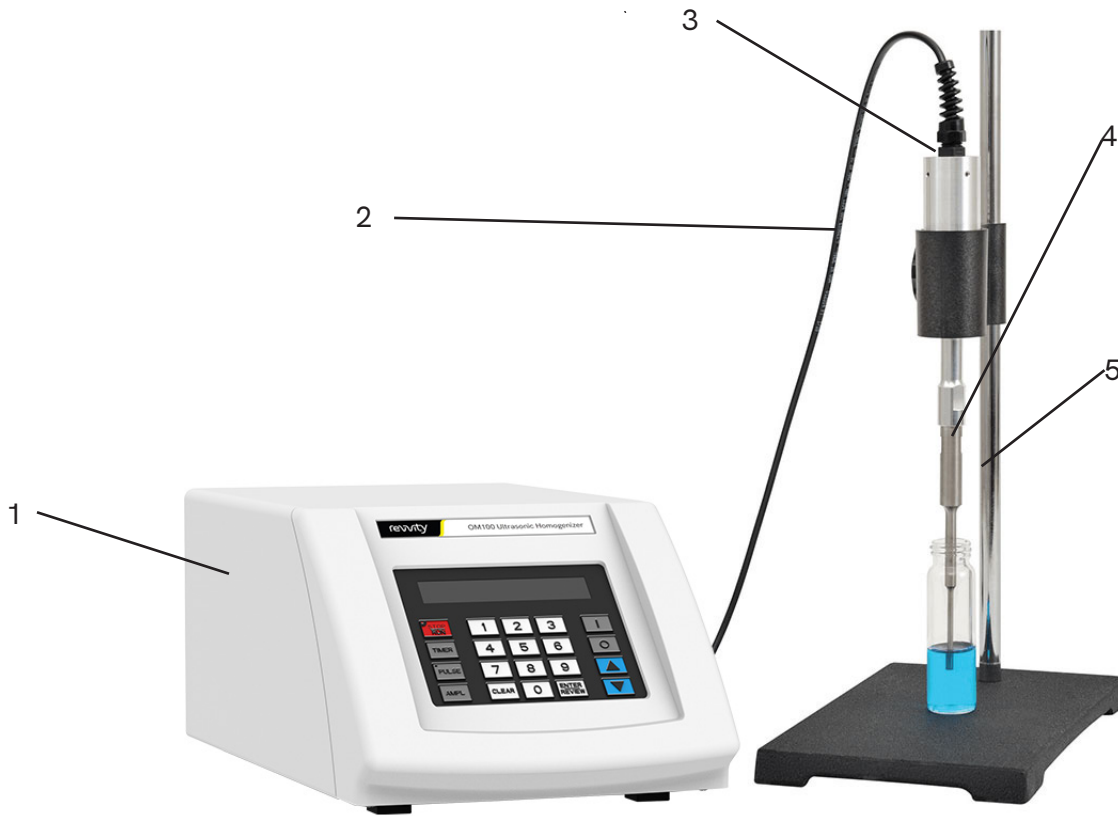
The OM100 ultrasonic homogenizer was designed to deliver constant amplitude to your liquid sample, regardless of these changes in load (much like the vehicle's cruise control described above). As a liquid is processed, the load on the probe will vary due to changes in the liquid sample (i.e., viscosity, concentration, temperature, etc.). As the resistance to the movement of the probe increases (increased load on the probe), additional power will be delivered by the power supply to ensure that the excursion at the probe tip remains constant. The displayed wattage readings will vary as the load changes; however, the amplitude will remain the same.

The resistance to the movement of the probe determines how much power will be delivered to maintain amplitude. For example, a 1/2" probe at 100% amplitude will require approximately 5 watts to operate in air. The amplitude of this probe is approximately 120um. Insert the probe in water and the wattage reading will increase to approximately 90 watts. The wattage required to operate the probe will increase as the load increases, but the amplitude remains the same.


The amplitude control allows the ultrasonic vibrations at the probe tip to be set to any desired level. Although the degree of cavitation/ultrasonic energy required to process the sample can readily be determined by visual observation, the amount of power required cannot be predetermined. A sensing network continuously monitors the output requirements, and automatically adjusts the power to maintain the amplitude at the preselected level. The greater the resistance to the movement of the probe due to higher viscosity, deeper immersion of the probe into the sample, larger probe diameter or higher pressure, the greater the amount of power that will be delivered to the probe. Setting the amplitude control to its maximum will not cause the maximum power rating of the unit to be delivered to the sample. The maximum power (100 watts) that the sonicator is capable of delivering will only be delivered when the resistance to the movement of the probe is high enough to draw the maximum wattage.

It is the intensity of cavitation that measures the effectiveness of sonication, not the total power applied to the system. Intensity is related to the amplitude of the radiating face of the tip or horn. It is amplitude that must be provided, maintained, and monitored. The unit provides controlled amplitude under varying load conditions to give reproducible results.

System Overview



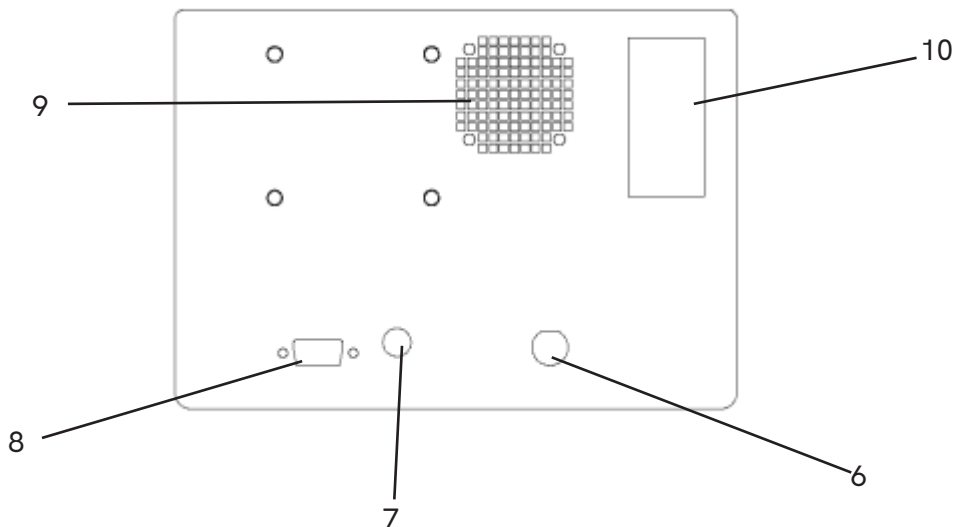
- 1. Power Supply
- 2. Convertor Cable
- 3. Convertor
- 4. Probe
- 5. Lab Stand with Clamp
- 6. Convertor Cable Connector
- 7. Footswitch Jack
- 8. Nine Pin Connector
- 9. Cooling Fan
- 10. Power Cord Connector



Functions Key Controls and Connectors

Front Panel	
LCD display	Displays prompts and the following control parameters: <ul style="list-style-type: none"> ▪ Amplitude selected ▪ Amount of output power delivered to the probe in watts, and as a percentage of 125 watts. ▪ Accumulated amount of energy in Joules delivered to the probe.
CLEAR key	Clears the preceding entry.
ENTER REVIEW key	Used to enter the amplitude selected, and view amplitude, power, and energy
START/STOP key	Starts or stops the OM100 ultrasonics. In the STOP mode the red indicator goes off.
I key	Switches the main power on.
0 key	Switches the main power off.
TIMER key	Used with the numeric keys to set the duration of ultrasonic application - from 1second to 9 hours, 59 minutes, 59 seconds.
PULSE key	Used with the numeric keys to set the pulse mode. The ON cycle and OFF cycle can be set independently from 1 second to 59 seconds. Red indicator lights when pulser is in the OFF portion of the cycle.
AMPL key	Controls the amplitude of vibration at the probe tip.
□ □ key	Used with the AMPL key when the unit is on stand-by to set the amplitude of vibration at the probe tip. Also used to increase or decrease the amplitude in small increments while the unit is running. To accomplish this task, depress the ENTER/REVIEW key twice to display AMPLITUDE CONTROL, then depress the □ or □ key as required.

Back Panel	
9 pin D-sub connector (IO Port)	Connects to external actuation device, and enable power and frequency monitoring.
Footswitch Connector	Connects to the footswitch cable.
Converter Cable Connector (Output)	Connects to the converter.
Power Supply Connector	Connects to the electrical line cord and encases the fuse(s).

9-Pin Sub Connector	
1	Not connected
2	Not connected
3	Not connected
4	Enables connection to a frequency counter.
5	Enables connection to external power monitor (5 mv = 1 watt)
6	Ground
7	Energizes the ultrasonics when connected to ground.
8 and 9	 <p>Enables the intensity to be remotely adjusted using an external 10k potentiometer.</p>

NOTE: To vary the intensity remotely using a variable DC power supply (0-5V) instead of a 10 K potentiometer, connect positive to pin 8 and negative to pin 6.

Convertor Clamping

Improper clamping can damage the system and void the warranty. Using a sound enclosure (part #060-12) or stand (part #060-10) will ensure a proper fit.



Proper Clamping



Improper Clamping

Preparation for Use

Inspection

Prior to installing the OM100 Ultrasonic Homogenizer, perform a visual inspection to detect any evidence of damage, which might have occurred during shipment. Before disposing of any packaging material, check it carefully for small items.

The OM100 Ultrasonic Homogenizer was carefully packed and thoroughly inspected before leaving our factory. The carrier, upon acceptance of the shipment, assumed responsibility for its safe delivery. Claims for loss or damage sustained in transit must be submitted to the carrier.

If damage has occurred, contact your carrier within 48 hours of the delivery date. **DO NOT OPERATE DAMAGED EQUIPMENT.** Retain all packing materials for future shipment.

Electrical Requirements

The OM100 Ultrasonic Homogenizer requires a fused, single phase 3-terminal grounding type electrical outlet capable of supplying 50/60 Hz at 100 volts, 115 volts, 220 volts, or 240 volts, depending on the voltage option selected. For power requirements, check the label on the back of the unit. Should it become necessary to convert the unit for different voltage operation, proceed as follows:

- Ensure that the power cord is not connected to the electrical outlet.
- Open the fuse holder cover using a small screwdriver.
- Pull out the red fuse holder from its housing.
- To convert from 100/115V to 220/240V replace the two 3 Amp slow blow fuses, with 1.6 Amp fuses.
- To convert from 220/240V to 100/115V reverse the procedure above.
- Rotate the fuse holder 180° from its original position, and reinsert it into its housing. For 100/115V operation the voltage displayed should be 115. For 220/240V operation the voltage display should be 220.
- Change the electrical power cord as required.
- Clearly note on the label or back of the unit that the voltage has changed.

WARNING: For your personal safety, do not, under any circumstances, defeat the grounding feature of the power cord by removing the grounding prong.

Installing the OM50 Ultrasonic Homogenizer

The OM100 Ultrasonic Homogenizer should be installed in an area that is free from excessive dust, dirt, explosive and corrosive fumes, and extremes of temperature and humidity. If processing flammable liquids use an approved fume hood and do not place the power supply in the fume hood.

When positioning the unit, be sure to leave adequate space behind the unit so that all connections can be easily disconnected.

Operating Instructions

- Do not operate continuously for more than 1 minute.
- Do not operate the power supply unless it is connected to the converter.
- Never allow liquid to spill into the converter.
- Do not allow a probe to vibrate in air for more than 10 seconds.
- Do not allow the vibrating probe to contact anything but the sample.
- Never place a washer between the probe and the converter.
- Never apply grease to the mating surfaces or threads of the converter or probe.
- Should it become necessary to remove a probe, use the wrenches supplied. Never attempt to remove the probe by twisting the converter housing, as this may damage the electrical connections within the housing.

NOTE: The temperature of the converter front area (where the probe attaches) should never exceed 60 °C (140 °F). If this temperature is reached, shut the system off and allow to cool.

Do not allow the system to operate for more than 1 minute without a rest or pulse to prevent overheating.

Setup

1. Plug the electrical line cord into the electrical outlet. If the unit is already on, depress the OFF key.
2. If the optional foot switch is used, insert the plug into the jack located on the rear panel.
3. Probes must be properly tightened. If the converter and probe assembly is not already assembled; screw the probe onto the converter and using the wrenches provided and tighten securely. Check the tightness of an already assembled probe by using the wrench set. Please refer to images in the Maintenance section of this manual for tightening instructions. A loose probe may cause damage to the power supply circuitry or parts of the converter and probe. Always use the wrenches supplied with the unit.
4. Sample processing should be used in pulse mode to prevent overheating - which could potentially crack the tip and damage the converter.
5. Probe tips wear after normal use. Using a severely worn probe tip can damage internal power supply components.
6. If using a laboratory stand, mount the converter/probe assembly using a clamp. Be sure to secure the clamp to the upper section of the converter housing only (see page 11).
7. Connect the converter cable to the power supply.
8. If the application requires long processing times we recommended chilling the sample and pulsing sonication.

Operation - Amplitude

Press the ON key. The screen will display the power rating of the OM100 Ultrasonic Homogenizer and the following control parameters.

```
Time - : --: --  
Pulse -- --           Ampl -- %
```

AMPLITUDE: Desired amplitude must be set in order for the OM100 Ultrasonic Homogenizer to be operational. The other control parameters – Time and Pulse, do not have to be set for continuous operation. AMPL displays the amplitude selected (e.g. 40%). To set the amplitude at 40% when the ultrasonics is off, press the AMPL key and the numeric keys for a 40% reading on the screen, and then press the ENTER/REVIEW key.

NOTE: The minimum amplitude setting is 20%.

The screen will display:

```
Time - : --: --  
  
NOTE: To clear an incorrect entry  
press the CLEAR key.
```

1. Immerse the probe approximately halfway into the sample. If the probe is immersed to an insufficient depth, air will be injected into the sample, causing the sample to foam. Also ensure that the probe tip is not touching the wall of the sample vessel.
2. The OM100 Ultrasonic Homogenizer is now ready for continuous operation. To energize the ultrasonics, press the START key or the footswitch. To de-energize the ultrasonics, press the STOP key or release the footswitch. If the Time or Pulse functions must be used, refer to the appropriate paragraphs below.

NOTE: The START key and footswitch are mutually exclusive. If the process is initiated by the START key, the footswitch becomes inoperative. If the process is initiated by the footswitch, the STOP key becomes inoperative.

3. To increase or decrease the amplitude in small increments when the ultrasonics is on, depress the AMPL to display Amplitude Setting on the screen, then depress the \square or \square key, as required. Since the amplitude required is application dependent and subject to the volume and composition of the sample, it is recommended that the amplitude be selected through experimentation, by increasing or decreasing the level of intensity as needed to properly process the sample to achieve desired results.

Operation - Timer

TIMER - In the pulsed mode the processing time will be different from the elapsed time because the processing time function monitors and controls only the ON portion of the duty cycle. For example, for 1 hour processing time, the elapsed time will be 2 hours if the ON and OFF cycle are set for 1 second.

1. To set the processing time, press the TIMER key. The screen will display:

```
Time Setting  
Hrs: - Min: -- Sec: --
```

2. Using the numeric keys, set the processing time as required, for example:

```
Time Setting  
Hrs: 0 Min: 10 Sec: 00
```

3. Press the ENTER/REVIEW key. The screen will display:

```
Time 0:10:00  
Pulse -- --           Ampl 40 %
```

Operation - Pulser

PULSER: Ultrasonics generates heat. Pulsing ultrasonics on and off helps to prevent heat build-up in temperature sensitive samples. In addition, pulsing may enhance processing by allowing the material to settle back under the probe after each burst. The ON and OFF pulse duration can be set independently from 01 second to 59 seconds. During the OFF portion of the cycle, the red indicator on the PULSE key will illuminate. If the OFF portion of the cycle exceeds three seconds, a cautionary message - Sonics in OFF Cycle - will warn the operator against touching the ultrasonic probe.

1. To set the pulser, press PULSE key. The screen will display:

Pulse on -- sec Pulse off --sec

2. Using the numeric keys, set the ON portion of the cycle and press the ENTER/REVIEW key. The screen will display:

Pulse on 05 sec Pulse off -- sec

3. Using the numeric keys set the OFF portion of the cycle. The screen will display:

Pulse on 05 sec Pulse off 05 sec

4. Press the ENTER/REVIEW key. The screen will display:

Time 0:10:00 Pulse 05 05 Ampl 40 %
--

Operation - Review

REVIEW: The REVIEW function provides a "window" on the process by displaying various operating parameters without process interruption. Pressing the ENTER/REVIEW key repeatedly during processing will consecutively display the following information.

Selected amplitude: e.g. Amplitude 40%

Selected processing time and elapsed processing time: e.g. Set 0:10:00 Time 0:05:00

Selected pulsing cycle and actual pulsing cycle: e.g. Pulse 05 05 / 05 00

Amount of power in watts, and accumulated amount of energy in JOULES delivered to the probe: e.g. 20 watts
0000000 Joules

NOTE: The amount of energy displayed will be only for one cycle. Initiating a new cycle will reset the display to zero.)

Elapsed time since processing was initiated: e.g. Elapsed time 0:05:00

Maintenance

It is recommended to periodically inspect the unit, both visually and physically, to ensure optimum and safe performance. This inspection should be scheduled as a routine maintenance procedure, done with the unit power OFF and with the unit unplugged from the AC power source.

Long exposure to acids or caustics results in corrosion of metal parts or components. Check the power supply, converter, and cables periodically for any signs of rust or discoloration. If discoloration is found, move the unit away from the source of the contaminant.

Examine the condition of the high voltage cable that attaches the converter to the generator. Inspect the wire insulation for damage, such as wear, burning from hot plate contact or breakage from extended use or rough handling. In general use, the cable assembly should not be used to carry the converter or pull it toward the user. Make certain the cable always has slack and is never tensioned. If necessary, move the generator or converter assembly closer to one another to accomplish this.

WARNING: Do not use a cable with broken end connections, exposed wires or frayed insulation. High voltage is present in the cable and will pose a shock hazard. Do not touch the converter assembly until the power switch is off and the unit is unplugged.

Probe Maintenance

Ultrasonic homogenizers create high intensity vibration which puts stress on the converter and horn assembly. The sides and end of the probe must never be allowed to come in contact with anything but the solution. When using a probe, the stress resulting at the point of contact with the vessel could cause the small probe tip to fracture.

Proper care of the probe is essential for dependable operation. The intense cavitation will, after usage for period of time, cause the tip to erode, and the power output to decrease. The smoother and shinier the tip, the more power will be transmitted into the sample. The vibrations may also cause the probe tip to loosen over time or the threaded connection to accumulate debris.

NOTE: A loose probe will usually generate a loud piercing or squealing sound.

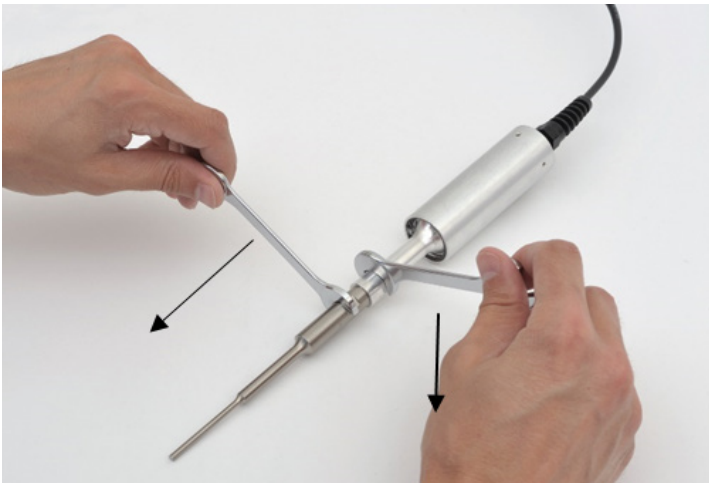
For that reason, it is recommended that a preventative maintenance schedule be adopted to examine the unit at regular intervals. The schedule should depend on frequency of use. Weekly maintenance schedules are recommended for units used frequently or monthly for those used infrequently. The tip must be examined for excessive wear and to ensure that the threaded connection is clean and attached properly to the converter. Use a cotton swab and alcohol (i.e. ethanol, isopropyl, etc.) to clean the threaded mating surfaces.

When excessive wear (corrosion/pitting of the probe tip) is detected the probe should be replaced with a new one.

WARNING: Probes must be properly tightened with the appropriate Wrench Set.

Attaching and Detaching Probes

1. Disconnect probe from converter. Use the wrench set provided with the system.
2. Clean threaded stud. Use alcohol and a cotton swab to remove any debris on the threading of the connecting stud. Allow the alcohol to dry completely.
3. Clean threading in converter. Use alcohol and a cotton swab to remove any debris on the threading. Do not allow liquid to drip into converter. Allow the alcohol to dry completely.
4. Re-attach probe to converter. Screw the probe back onto the converter and tighten with the wrench set provided.



System Cleaning Instructions

The power supply and converter may be cleaned using an acid-free cleaning solution (i.e. glass cleaner).

Probes should be cleaned using isopropyl alcohol. Probes are made from titanium and can be autoclaved (the converter is an electrical part and cannot be sterilized in this manner). Before each procedure place the probe tip in water or alcohol and turn the power on for a few seconds to remove residue. The tip also can be sterilized using alcohol with the power on.

Troubleshooting

The most probable causes for malfunction are listed below and should be investigated.

- A connector or cable is damaged.
- The unit was plugged into an electrical outlet that provides a different voltage from that required. See Electrical Requirements.
- The probe is not tightened properly with the wrenches provided.
- The converter and/or probe has been dropped.
- A probe being operated is damaged or worn past its useful life.
- A fuse(s) has failed. If a fuse(s) has failed, proceed as follows:
 1. Turn the unit off by depressing the OFF key, and disconnect the line cord from the electrical outlet.
 2. Open the fuse holder cover using a small screwdriver, and pull out the red fuse holder from its housing.
 3. Replace the fuse(s).
 4. Reconnect the line cord to the electrical outlet, press the ON key and set the amplitude to 100. With the probe in air (out of the sample), the wattmeter should read below 10 watts. If the reading exceeds 10 watts, press the OFF key, and disconnect the probe from the converter.
 5. Press the ON key. If the wattmeter reads below 10 watts, the probe has failed or is out of tune due to excessive erosion, and should be replaced, if the wattmeter reads above 20 watts, either the converter or power supply has failed and the complete OM100 Ultrasonic Homogenizer should be returned for repair.

Overload Condition

If the OM100 Ultrasonic Homogenizer stops working, and an OVERLOAD indication is displayed on the screen, check for possible causes as outlined in the above paragraph, then press the OFF key to switch the unit off, and the ON key to switch the unit back on.

If the problem persists after inspecting all of these, please contact Customer Service for additional assistance or to replace a worn probe or damaged part.

Frequently Asked Questions

Probe Size versus Sample Volume

Selecting the proper size probe is a critical factor when sonicating a sample. The sample volume to be processed must correlate with the tip diameter. Each probe has a recommended sample volume range. This range may overlap with other probes.

For example the 1/8" probe is recommended for approximately 500 µL to 15 mL.

Depending on the application and type of sample, you may be able to process a volume outside of our recommended range.

Small volumes require a small tip diameter. Small probes (1/4" or less) are recommended for processing samples inside small, thin vessels such as microcentrifuge tubes. These small probe sizes are high intensity and made for short processing times. Using a small probe tip for long time periods will generate a considerable amount of heat. Pulse mode should be used to reduce heat buildup.

While there is no absolute sample volume range for any probe/horn, below is a general guideline to follow. Using a sample volume outside each tip diameter's range is normally not recommended. Processing volumes are application specific.

Tip Diameter	Processing Volume Range
5/64" (1.6 mm)	200 µL to 5 mL
1/8" (3.2 mm)	500 µL to 15 mL
1/4" (6.4 mm)	10 mL to 50 mL

Vessel Shape and Size

A narrow vessel is preferable to a wide vessel. The ultrasonic energy is generated from the tip and is directed downward. As a sample is processed the liquid is pushed down and away in all directions. If the vessel is too wide, it will not mix effectively and some sample will remain untreated at the periphery. The probe should never touch the sides or bottom of the vessel.

How to Prevent Foaming (Small Sample Issue)

Foaming is a problem that often occurs with samples volumes below 1ml. The cause of foaming is generally 3 issues: amplitude is too high for a small volume, tip is too large for the volume, or the tip is not inserted to a proper depth.

Tip depth

The depth of the probe within the liquid is an important issue. If the probe is too close to the surface of the liquid, it can create foam. If the probe is too deep, it may sonicate against the bottom of the vessel and not effectively processing the sample. The sample must flow freely below the tip in order to be mixed effectively.

Without effective mixing you cannot ensure the entire sample volume will pass below the tip and become processed. The probe should be submerged approximately halfway into the liquid but there are exceptions. Before processing actual samples, it is recommended to test the probe in a vessel filled with water to observe the ultrasonic energy and the flow pattern of the liquid. During this test you can adjust the probe's depth until you see adequate mixing and movement of the water.

Power versus Intensity

Power is the measure of the electrical energy that is being delivered to the converter. It is measured in watts and displayed on the sonicator's screen. At the converter, the electrical energy is transformed into mechanical energy. It does this by exciting the piezoelectric crystals causing them to move in the longitudinal direction within the convertor. This change from electrical into mechanical energy causes a motion that travels through the horn/probe causing the tip to move up and down.

The distance of one movement up and down is called its amplitude. The amplitude is adjustable. Each probe has a maximum amplitude value. For example, with a 1/8" diameter probe at setting 100%, the probe will achieve an amplitude of approximately 180µm. At setting 50% the amplitude is approximately 90µm.

NOTE: This is approximate and not perfectly linear. We measure the amplitude of each probe at 100% and these values are published in the brochure.

Amplitude and intensity have a direct relationship. If you operate at a low amplitude setting, you will deliver low intensity sonication. If you operate at a high amplitude setting, you will have high intensity sonication. In order to be able to reproduce results, the amplitude setting, temperature, viscosity and volume of the sample are all parameters that need to remain consistent. The amplitude, not the power, is most critical when trying to reproduce sonication results.

Power has a variable relationship with amplitude/intensity. For example, sonicating water requires less wattage when compared to a viscous sample (such as oil). While sonicating both samples at the same amplitude setting the power/wattage will differ because the viscous sample will require more watts in order to drive the horn. The viscous sample puts a heavier load on the probe so they system must work harder to vibrate up and down at the same amplitude setting. The oil may draw double the watts when operated at the same amplitude as the water sample.

Small fluctuation in the wattage during sonication is normal. Major swings in wattage (+/- 20 watts) may indicate a problem with the sample, setup or the sonicator itself.

Viscosity Limitations

Viscous solutions and highly concentrated liquids can be difficult to sonicate. If the liquid is so thick that it cannot be easily poured out of a vessel it is likely too viscous to be sonicated.

Keeping Samples Cool

Ultrasonic processing causes the liquid temperature to elevate especially with small volumes. Pulsed sonication is always recommended. The addition of an ice bath or recirculating chiller to cool the sample vessel is strongly suggested.

Accessories

Part Number	Description
060-078	5/64" (2 mm) Tip Diameter Probe
060-125	1/8" (3.2 mm) Tip Diameter Probe
060-250	1/4" (6.4 mm) Tip Diameter Probe
060-10	Support Stand with Converter Holder for OM50 and OM100
060-12	Sound Enclosure with Converter Holder for OM50 and OM100
060-13	Replacement Converter for OM100

Appendix

Transport and Storage

Permissible environmental conditions for transport and storage of the equipment:

- Temperature 35°F to 120°F / 2°C to 49°C
- Relative Humidity 10 % to 95 % (Non Condensing)
- Altitude 40,000 ft. (12,192 m)

Equipment Disposal

This equipment is marked with the crossed-out wheeled bin symbol, to indicate that this equipment may not be disposed of as unsorted municipal waste.

It's your responsibility to correctly dispose of your equipment at life-cycle end, by handing it over to an authorized facility for separate collection and recycling of waste equipment. It's also your responsibility to decontaminate your equipment in case of biological, chemical or radiological contamination, and so protect the persons involved in the disposal and recycling of the equipment from health hazards.

For more information about where you can dispose of your waste equipment, please contact your local dealer, from whom you purchased the equipment.

By doing so, you will help to preserve natural and environmental resources and you will ensure that your equipment is recycled in a manner that protects human health.



This page left blank intentionally.

This page left blank intentionally.



The information provided in this document is for reference purposes only and may not be all-inclusive. Revvity, Inc., its subsidiaries, and/or affiliates (collectively, "Revvity") do not assume liability for the accuracy or completeness of the information contained herein. Users should exercise caution when handling materials as they may present unknown hazards. Revvity shall not be liable for any damages or losses resulting from handling or contact with the product, as Revvity cannot control actual methods, volumes, or conditions of use. Users are responsible for ensuring the product's suitability for their specific application. REVVITY EXPRESSLY DISCLAIMS ALL WARRANTIES, INCLUDING WARRANTIES OF MERCHANTABILITY OR FITNESS FOR A PARTICULAR PURPOSE, REGARDLESS OF WHETHER ORAL OR WRITTEN, EXPRESS OR IMPLIED, ALLEGEDLY ARISING FROM ANY USAGE OF ANY TRADE OR ANY COURSE OF DEALING IN CONNECTION WITH THE USE OF INFORMATION CONTAINED HEREIN OR THE PRODUCT ITSELF.

www.revvity.com

revvity

For research use only. Not for use in therapeutic or diagnostic procedures

Revvity, Inc.
940 Winter Street
Waltham, MA 02451
USA
www.revvity.com

For a complete listing of our global offices, visit www.revvity.com
Copyright ©2024, Revvity, Inc. All rights reserved.